KNAUER

AZURA

AZURA Compact Bio LC 50
Flow scheme

Example Configuration

1: Wash Buffer
2: Elution Buffer
3: Sample
4: CIP-Solution
5: Storage
6: Water

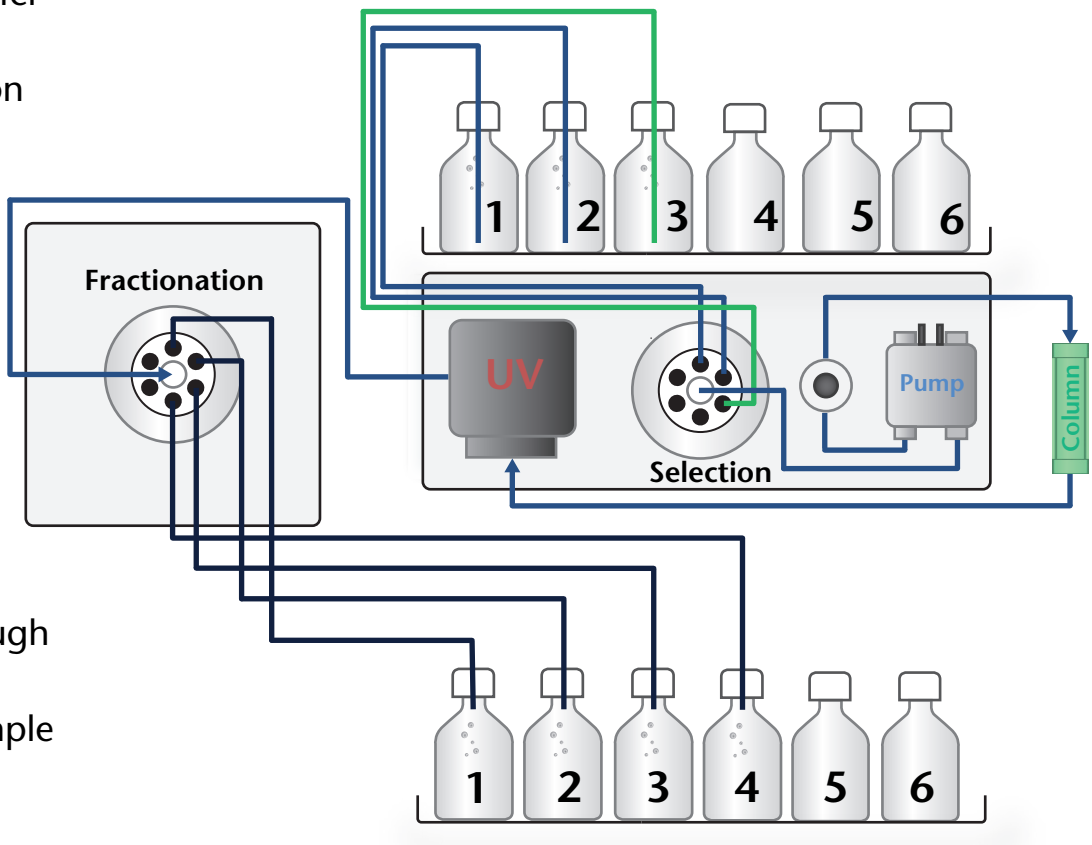

1: Waste
2: Flow Through
3: Wash
4: Eluted Sample
5: Optional
6: Optional

® AZURA
All rights reserved.

The information in this document is subject to change without prior notice.
Printed on environmentally friendly paper from sustainable forests.

Date of the last update: 27.11.2015
HPLC · SMB · Osmometrie

© KNAUER
Wissenschaftliche Geräte GmbH
Hegauer Weg 38
14163 Berlin, Germany

Phone: +49 30 809727-0
Telefax: +49 30 8015010
E-Mail: info@knauer.net
Internet: www.knauer.net